


scan to configure

scan for tutorial



I.O

TECHNICAL SCHEME

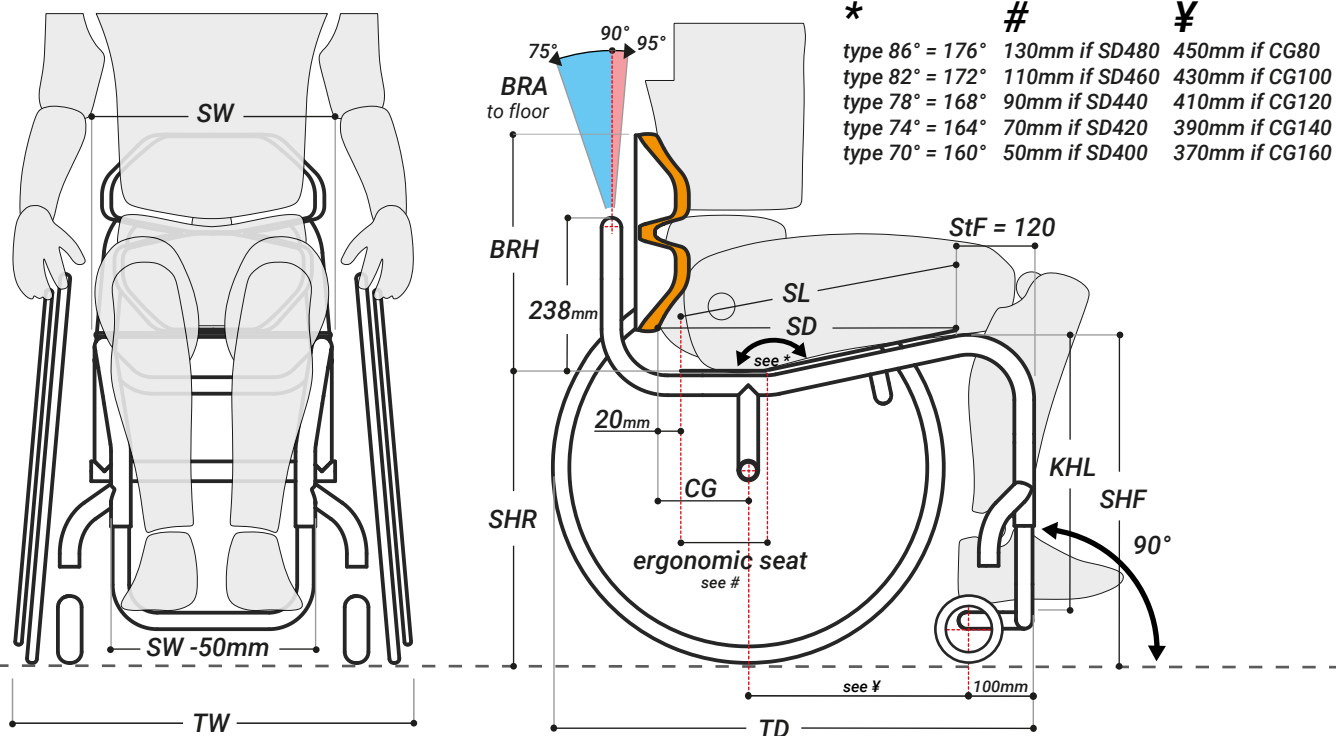

The technical scheme do not consider the dimensions of any postural and anti decubitus cushions.

SW: Considered external tube to external tube of the frame. The dimension between the internal faces of the side guards is +10 mm than the SW.

SD: Considered the depth of the seat. It considers the dimension from the end of the seat to the postural backrest.

SL: Considered the length of the seat pan. SL with CARBFX = SD - 20mm | SL with CARBTF = SD - 20mm

CG: Considered from the backrest foam to the axle of the rear wheels.

StF: The value 120mm of the StF is fixed and cannot be modified.

BRH: Considered from the seat (upholstery or carbon) to the top of the backrest.

TOLERANCE: The product is manufactured with a tolerance of ± 5 mm

Backrest foam, thickness 30 mm.

For a right sizing of the wheelchair is recommended:

SW | Seat Width _ A space of ± 5 mm between the user basin and the side guards.

SD | Seat Depth _ A space of ± 50 mm between the user's popliteal fossa and the seat.



SW: 340 – 440 mm
in increments
of 20 mm



SD: 400 – 480 mm
in increments
of 20 mm



BRH: 255 – 405 mm
in increments
of 15 mm



SHR: 360 – 500 mm
in increments
of 10 mm



SHF: 460 – 520 mm
in increments
of 10 mm



KHL: 310 – 420 mm
in increments
of 10 mm



CG: 80 – 160 mm
in increments
of 20 mm



BRA: 85° - 95°
in increments
of 1°



CRW:
0° or 3°



TOTAL WIDTH (TW)
(Camber 0°)
SW + 195 mm
(Camber 3°)
SW + 240 mm



TOTAL DEPTH (TD)
StF + SD + 80 + 100
+ (100-CG)



TRASPOT WEIGHT
(Without rear wheels
and backrest)
 ± 4.9 kg*



**MAXIMUM
USER WEIGHT**
120 Kg



*** CONFIGURATION:**
SW340 / SD420 / STF120 /
BRH255 / FOOT1 /
BRKASL / FRKDS2 /
FRWH4 / CARB3 / BKR1F /
RT1 / FONOT / CARB73

ARIA WHEELS SRL

Registered Office_Via della Divisione Torino, 92 00143 Roma - Italy

Production Dept_Via A. Volta, 7/B 36030 Costabissara (VI) - Italy

VAT IT 12848301003 | tel.+39 0444701414

www.ariawheels.com | info@ariawheels.com